


Chromatogram and Results

Injection Details

| | | | |
|----------------------|----------------------|-------------------|----------|
| Injection Name: | RAD140; BA34101 | Run Time (min): | 20.00 |
| Vial Number: | | Injection Volume: | 10.00 |
| Injection Type: | Unknown | Channel: | EXT278NM |
| Calibration Level: | | Wavelength: | n.a. |
| Instrument Method: | AD 150mm MaxRP 20min | Bandwidth: | n.a. |
| Processing Method: | Processing Method | Dilution Factor: | 1.0000 |
| Injection Date/Time: | 27/Apr/25 15:26 | Sample Weight: | 1.0000 |

Chromatogram

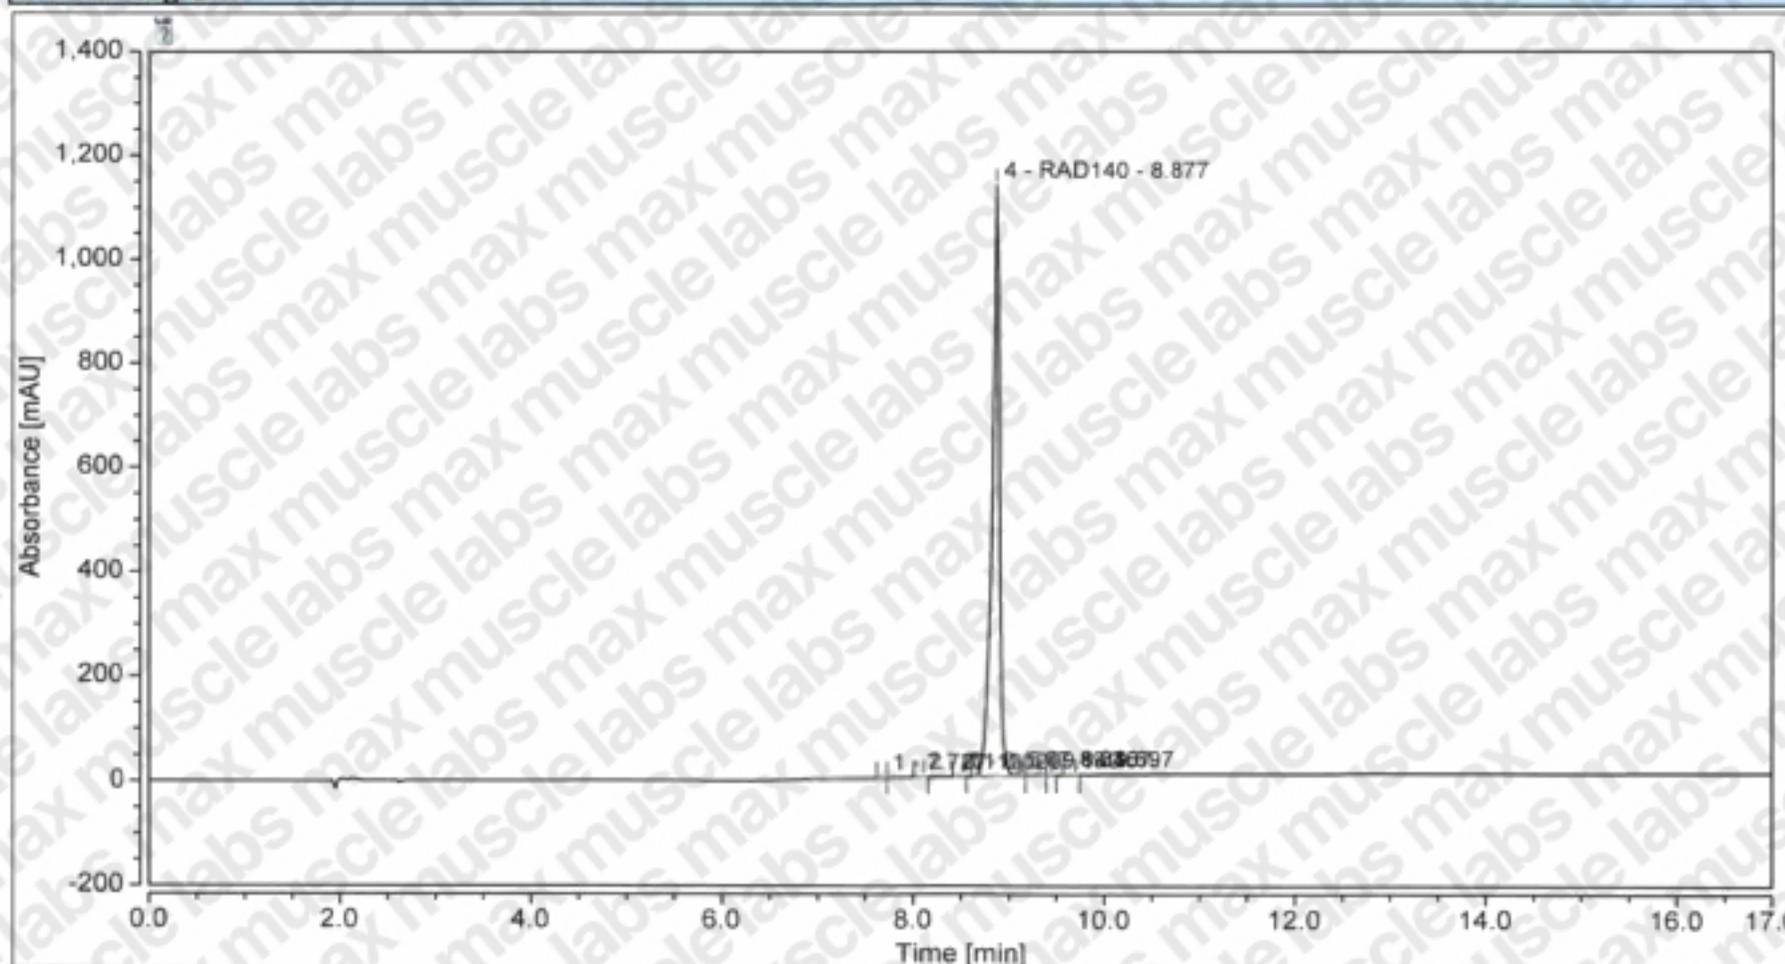

Integration Results

| No. | Peak Name | Retention Time min | Area mAU*min | Height mAU | Relative Area % | Relative Height % | Amount |
|---------------|-----------|-----------------------|-----------------|-----------------|--------------------|----------------------|--------|
| 1 | | 7.727 | 0.005 | 0.000 | 0.01 | 0.00 | n.a. |
| 2 | | 8.113 | 0.016 | 0.253 | 0.02 | 0.02 | n.a. |
| 3 | | 8.520 | 0.011 | 0.117 | 0.01 | 0.01 | n.a. |
| 4 | RAD140 | 8.877 | 98.888 | 1133.804 | 99.77 | 99.71 | n.a. |
| 5 | | 9.140 | 0.006 | 0.152 | 0.01 | 0.01 | n.a. |
| 6 | | 9.330 | 0.142 | 1.984 | 0.14 | 0.17 | n.a. |
| 7 | | 9.457 | 0.016 | 0.337 | 0.02 | 0.03 | n.a. |
| 8 | | 9.697 | 0.028 | 0.419 | 0.03 | 0.04 | n.a. |
| Total: | | | 99.112 | 1137.066 | 100.00 | 100.00 | |