


Chromatogram and Results

Injection Details

Injection Name:	ACP105; BA34701	Run Time (min):	25.00
Vial Number:		Injection Volume:	10.00
Injection Type:	Unknown	Channel:	UV_VIS_1
Calibration Level:		Wavelength:	195
Instrument Method:	AD 250mm MaxRP 25min Purity Method	Bandwidth:	5
Processing Method:	Processing Method	Dilution Factor:	1.0000
Injection Date/Time:	14/Mar/25 12:33	Sample Weight:	1.0000

Chromatogram

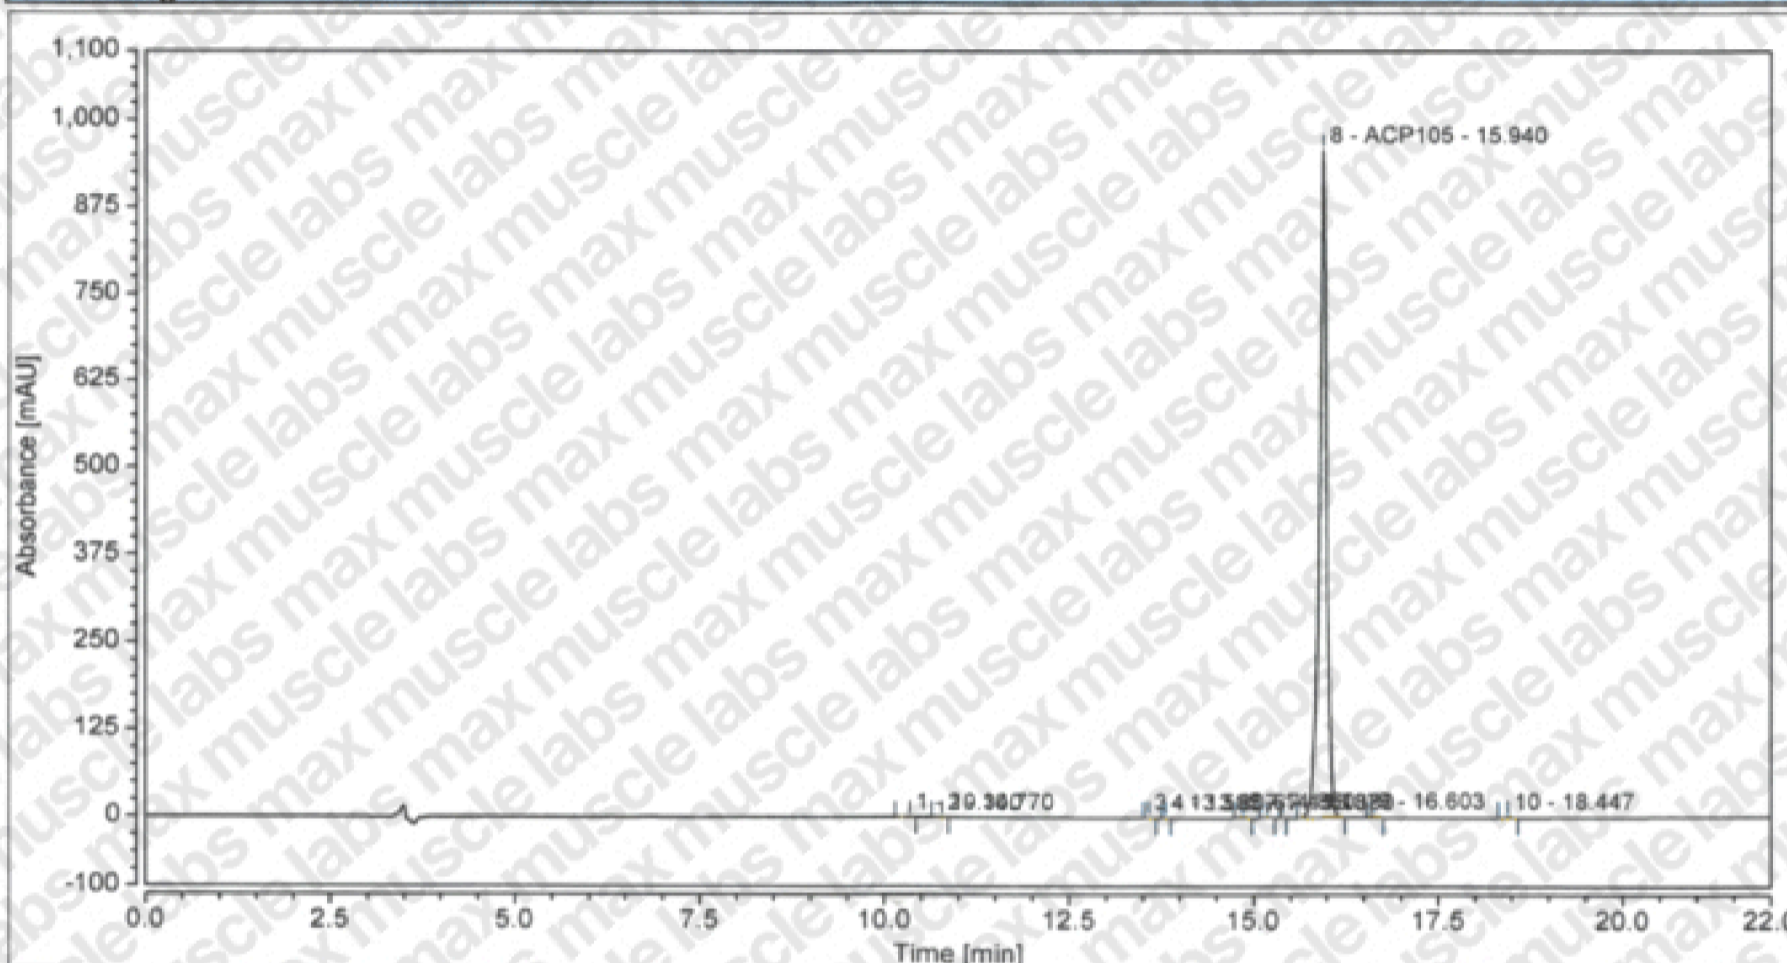

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1		10.340	0.036	0.244	0.03	0.03	n.a.
2		10.770	0.024	0.202	0.02	0.02	n.a.
3		13.583	0.022	0.310	0.02	0.03	n.a.
4		13.807	0.007	0.129	0.01	0.01	n.a.
5		14.850	0.146	1.506	0.13	0.16	n.a.
6		15.187	0.053	0.612	0.05	0.06	n.a.
7		15.380	0.010	0.205	0.01	0.02	n.a.
8	ACP105	15.940	113.693	957.227	99.50	99.37	n.a.
9		16.603	0.145	1.618	0.13	0.17	n.a.
10		18.447	0.126	1.289	0.11	0.13	n.a.
Total:			114.263	963.340	100.00	100.00	